

Amersham™
ECL Select™ Western Blotting
Detection Reagent

Product booklet

Code: RPN2235



Page Finder

1. Legal	4
2. Description	5
2.1 Introduction	5
2.2 Design and features	6
2.3 Compatibility	6
3. Important user information	7
3.1 Intended use	7
3.2 Safety notices	7
3.3 Quality control	7
4. Handling	8
4.1 Safety precautions	8
4.2 Storage	8
4.3 Expiry	8
5. Required components	9
5.1 Kit components	9
5.2 Solutions	9
5.3 Membrane	9
5.4 Blocking reagents	9
5.5 Immunodetection reagents	10
6. Western blotting optimization	10
6.1 Molecular weight markers	11
6.2 Membranes	11
6.3 Transfer	12
6.4 Blocking	12
6.5 Imagers and film	13
6.6 Western blotting handbook	13
7. Protocol	14
7.1 Electrophoresis and transfer	15

7.2	Blocking	15
7.3	Antibody probing	15
7.4	Dilution ranges	16
7.5	Primary antibody incubation	16
7.6	Secondary antibody incubation	17
7.7	Streptavidin bridge incubation	18
7.8	Detection	18
7.9	Image analysis	19
7.10	CCD camera	19
7.11	X-ray film	20
8.	Additional information	21
8.1	Stripping and reprobing membranes	21
8.2	Determination of optimum antibody concentration	22
8.3	Dilution ranges	22
8.4	Primary antibody optimization	22
8.5	Secondary antibody optimization	24
9.	Troubleshooting guide	25
10.	Related products	27
10.1	Sample preparation	28
10.2	Molecular weight markers	28
10.3	Gel electrophoresis equipment	29
10.4	Transfer equipment	31
10.5	Blotting equipment	31
10.6	Blocking agents	32
10.7	ECL HRP-linked secondary antibodies	33
10.8	Detection reagents	34
10.9	ECL Plex CyDye conjugated antibodies	34
10.10	X-ray films	35
10.11	Imaging systems	35
10.12	Software and accessories	35

1. Legal

GE, the GE monogram, Imagination at work, Amersham, ECL, ECL DualVue, ECL Select, ECL Prime, Hybond, Hyperfilm, ImageQuant, Protran and Rainbow are trademarks of General Electric Company.

Amersham ECL Select is manufactured and sold under license from Cyanagen Srl and is subject of US Canadian and EU patent application number US7803573; EP1962095; US7855287; EP1950207 US2012009603(A1); CA2742025; EP2405016, together with other equivalent granted patents and patent applications in other countries.

Tween is a trademark of ICI Americas Inc.

All other third party trademarks are the property of their respective owner.

© 2006-2017 General Electric Company – All rights reserved.

Previously published February 2014

All goods and services are sold subject to the terms and conditions of sale of the company within GE Healthcare which supplies them.

A copy of these terms and conditions is available on request.

Contact your local GE Healthcare representative for the most current information.

<http://www.gelifesciences.com/ecl>

GE Healthcare UK Limited.


Amersham Place, Little Chalfont,
Buckinghamshire, HP7 9NA UK

2. Description

Amersham™ ECL Select™ Western blotting detection reagent from GE Healthcare provides very high sensitivity for chemiluminescent detection of immobilized specific antigens conjugated to Horseradish Peroxidase (HRP) labeled antibodies.

2.1 Introduction

Chemiluminescence is defined as light emission produced in a multistep reaction whereby peroxidase catalyzes the oxidation of luminol. In the presence of chemical enhancers and catalysts, the light intensity and the duration of light emission is greatly increased in a process known as enhanced chemiluminescence (ECL). ECL based on horseradish peroxidase (HRP)-conjugated secondary antibodies is a sensitive detection method where the light emission is proportional to protein quantity. The multi-step reaction is illustrated below.

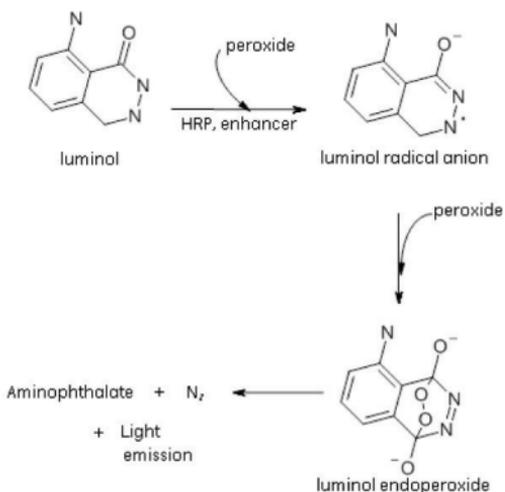

2.2 Design and features

Amersham ECL Select detection reagent is designed to provide very high light output. This means that medium to very low protein amounts (low picogram levels) can be detected using highly diluted antibodies. This makes Amersham ECL Select suitable for the most demanding Western blots regarding sensitivity requirements. The high signal intensity can fully utilize the advantages of CCD camera based imaging equipment and makes Amersham ECL Select optimal for detection with ImageQuant™ LAS systems from GE Healthcare. The output light can also be detected using X-ray film (Amersham Hyperfilm™ product range).

2.3 Compatibility

Amersham ECL Select detection reagent is compatible with PVDF and nitrocellulose membranes (such as Amersham Hybond™ and Amersham Protran product range), Amersham ECL Prime Blocking Agent, Amersham ECL Blocking Agent and other commonly used blocking agents such as BSA and non-fat dry milk.

3. Important user information

3.1 Intended use

Amersham ECL Select detection reagent is intended for chemiluminescent detection in Western blotting.

Amersham ECL Select detection reagent is intended for research use only, and shall not be used in any clinical procedures, or for diagnostic purposes.

3.2 Safety notices

This user documentation contains CAUTIONS concerning the safe use of Amersham ECL Select detection reagent. See definitions below.

Cautions



CAUTION

CAUTION indicates a hazardous situation which, if not avoided, could result in minor or moderate injury. It is important not to proceed until all stated conditions are met and clearly understood.

3.3 Quality control

Amersham ECL Select detection reagent is manufactured in compliance with our ISO 9001 certified quality management system, and is in conformity with the acceptance criteria set up for the product.

4. Handling

4.1 Safety precautions



CAUTION

Hazardous substances. When using hazardous chemicals, take all suitable protective measures, such as wearing protective glasses and gloves resistant to the substances used. Follow local and/or national regulations for safe operation.

It is recommended to read the Safety Data Sheet (SDS) before using Amersham ECL Select detection reagent.

4.2 Storage

On receipt, all components should be stored at 18–30°C. Amersham ECL Select detection reagent is sensitive to prolonged exposure to light. Always store the individual reagents in the light-tight containers in which they are provided.

4.3 Expiry

The components are stable for at least 3 months when stored under the recommended conditions. See expiry date on package.

5. Required components

5.1 Kit components

The following components are included in the Amersham ECL Select detection reagent kit.

Product	Content
RPN2235	<ul style="list-style-type: none">• Solution A: Luminol solution, 50 ml.• Solution B: Peroxide solution, 50 ml. Sufficient for 1000 cm ² membrane

5.2 Solutions

Required solutions are listed below.

- Phosphate buffered saline (PBS), pH 7.5
- Tris buffered saline (TBS), pH 7.6
- Dilution and wash buffer: PBS Tween™ (PBS-T) and TBS Tween (TBS-T). A Tween 20 concentration of 0.1% is suitable for most blotting applications.

5.3 Membrane

Use a suitable protocol to separate proteins by electrophoresis and transfer them to a PVDF or nitrocellulose membrane.

5.4 Blocking reagents

Blocking reagents are typically diluted to 2% to 5% (v/v) in PBS-T or TBS-T buffer. The following blocking reagents are recommended:

- Amersham ECL Prime Blocking Agent
- Amersham ECL Blocking Agent
- Non-fat dry milk
- Bovine Serum Albumin (BSA)

5.5 Immunodetection reagents

- Primary antibody specific to the target protein(s)
- HRP conjugated secondary antibody specific to the primary antibody. See *ECL HRP-linked secondary antibodies*, on page 33.

Dilute the antibodies in PBS-T or TBS-T according to the recommendations in *Dilution ranges*, on page 22.

6. Western blotting optimization

Introduction

To achieve an optimal Western blotting result with high signal to noise ratio and best possible sensitivity and linearity, it is important to optimize the method and to select compatible products.

Consider the following:

- **Sample quality and loading amount** – It is important that the sample is of good quality and that detectable levels of target protein is present.
- **Membrane and blocking** – Select membranes and blocking agents compatible with sample and antibodies.
- **Primary and secondary antibodies** – Always select specific antibodies of high quality and optimize the antibody dilution.
- **Detection and imaging** – Select detection reagent according to your application need. A CCD imager offers high sensitivity and broad dynamic range and provide better quantification than X-ray film.

This chapter describes products recommended for use with Amersham ECL Select detection reagent. For more information regarding these products, refer to www.gelifesciences.com/ecl.

6.1 Molecular weight markers

Molecular weight markers are used to determine protein size. In addition, pre-stained markers allow confirmation of protein transfer and orientation (as the colored bands transfer to the membrane).

- **Amersham Rainbow™ Markers** are pre-stained multicolored markers for monitoring progress of protein electrophoresis, confirming transfer efficiency and determination of molecular weight of blotted proteins.
- **Amersham ECL DualVue™ Markers** are markers optimized for use with Amersham ECL, Amersham ECL Prime and Amersham ECL Select and contains a combination of pre-stained and tagged proteins markers. These markers enable monitoring of electrophoresis, confirming transfer efficiency and determination of molecular weight of blotted proteins without staining on gel and membrane, as well as in chemiluminescence detection.

6.2 Membranes

- **Amersham Hybond** is a PVDF membrane with high protein binding capacity and mechanical strength, which makes it ideal for Western blotting applications where stripping and re-probing are needed. The membrane is optimal for use with Amersham ECL Prime and ECL Select detection reagents.
- **Amersham Protran** is a nitrocellulose membrane compatible with all chemiluminescent Western blotting substrates. The main advantage is the normally low background.

6.3 Transfer

- **Wet transfer** (Transfer Unit TE 22), is the most commonly used transfer method. It provides efficient transfer of small to large proteins.
- **Semi-dry transfer** (Transfer Units TE 70 and TE 77), is faster than wet transfer and consumes less buffer. Semi-dry transfer works well for most proteins but transfer may be less efficient for large proteins. It might have reduced sensitivity for very low abundance proteins.

6.4 Blocking

After protein transfer the membrane need to be incubated in a blocking solution to prevent non-specific binding of antibodies, which can cause background and non-specific protein bands on the blot. The blocking agent should be optimized for best results, no single blocking agent is optimal for all proteins and antibodies. GE Healthcare recommend the following blocking agents compatible with Amersham ECL, Amersham ECL Prime and Amersham ECL Select:

- **Amersham ECL Prime Blocking Agent**
- **Amersham ECL Blocking Agent**
- **BSA Blocking Agent**
- **Non-fat dry milk**

6.5 Imagers and film

The **ImageQuant LAS systems** are flexible systems that cover a wide range of imaging applications. These CCD based imagers provide an affordable option for protein detection with genuine benefits, including quantitation with high sensitivity, publication grade data, and image and data archiving.



ImageQuant LAS 500

Amersham Hyperfilm product range are trusted products for sensitive, qualitative chemiluminescent detection in Western blots.


6.6 Western blotting handbook

More technical help, tips, and best practices can be found in the handbook *Western Blotting Principles and Methods* from GE Healthcare (code no. 28-9998-97).

7. Protocol

Protocol overview

Below is an overview of the Western blotting detection protocol.

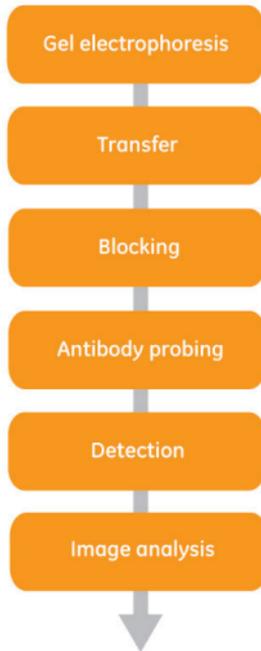

7.1 Electrophoresis and transfer

Step	Action
------	--------

1. Perform electrophoresis and transfer proteins to a suitable membrane according to standard protocols. Blots are preferably used immediately but may be stored in PBS-T or TBS-T at 2°C to 8°C.

Note: *Amersham Hybond membrane should be pre-wetted in 100% methanol prior to equilibration in transfer buffer.*

7.2 Blocking

Step	Action
------	--------

1. Incubate the membrane in a suitable blocking solution on an orbital shaker for 1 hour at room temperature or overnight at 2°C to 8°C.
2. Briefly rinse the membrane with two changes of wash buffer.

Note: *For preparation of wash buffer, see Solutions, on page 9.*

7.3 Antibody probing

Amersham ECL Select detection reagent has very high light output and therefore allows high antibody dilutions. The optimal dilution varies between antibodies depending on affinity and quality.

Optimization of the antibody dilution can be performed by dot blot analysis (see *Determination of optimum antibody concentration, on page 22*).

7.4 Dilution ranges

The following dilution ranges are recommended:

Antibody	Dilution range from 1 mg/ml stock solution
Primary	1:5000 - 1:30000
Secondary	1:100000 - 1:300000

The table below shows suggested starting dilutions for primary antibodies with different levels of affinity.

Type of antibody	Primary antibody dilution	Secondary antibody dilution
High affinity primary antibodies	1:10000	1:150000
Medium to low affinity primary antibodies	1:5000	1:100000

7.5 Primary antibody incubation

Step	Action
------	--------

1. Dilute the primary antibody in PBS-T or TBS-T.
2. Incubate the membrane in the primary antibody solution on an orbital shaker for 1 hour at room temperature or overnight at 2°C to 8°C.
3. Briefly rinse the membrane with two changes of wash buffer.
4. Wash the membrane 4 to 6 times in wash buffer for 5 minutes each at room temperature on an orbital shaker.
Note: Exposure to X-ray film requires 6 wash steps, to avoid background.

7.6 Secondary antibody incubation

Step	Action	Notes
1.	Dilute the secondary antibody (HRP conjugated or biotinylated antibody) in PBS-T or TBS-T.	Increase the light output by building a three layer sandwich using biotinylated secondary antibodies and HRP conjugated streptavidin.
2.	Incubate the membrane in the secondary antibody solution for 1 hour at room temperature on an orbital shaker.	
3.	Briefly rinse the membrane with two changes of wash buffer.	
4.	Wash the membrane 4 to 6 times in wash buffer for 5 minutes each at room temperature on an orbital shaker.	Exposure to film requires 6 wash steps, to avoid background.

If using an HRP conjugated secondary antibody, proceed directly to *Detection*, on page 18.

If using a biotinylated antibody, proceed with the streptavidin bridge incubation protocol overleaf.

7.7 Streptavidin bridge incubation

Step	Action
1.	Dilute the Streptavidin HRP conjugate or Streptavidin biotinylated HRP complex in PBS-T or TBS-T.
2.	Incubate the membrane in the diluted solution for 1 hour at room temperature on an orbital shaker.
3.	Briefly rinse the membrane with two changes of wash buffer.
4.	Wash the membrane by suspending it in enough wash buffer to cover the membrane and agitate for 5 minutes at room temperature. Replace wash buffer at least 4 to 6 times.



7.8 Detection

Step	Action
1.	Mix detection solutions A (luminol) and B (peroxide) in a ratio of 1:1 to a working solution. The final volume of detection reagent required is 0.1 ml/cm ² membrane. Note: <i>If the mixed reagent is not to be used immediately, protect it from exposure to the light either by wrapping in foil or storing in a dark place.</i>
2.	Drain the excess wash buffer from the washed membrane and place it protein side up in a suitable box or on a sheet of plastic wrap or other suitable clean surface. Add detection reagent onto the membrane and make sure it completely covers the membrane.
3.	Incubate for 5 minutes at room temperature.
4.	Drain off excess detection reagent by holding the membrane edge gently against a tissue.

7.9 Image analysis

Two protocols for image analysis are described, one for CCD camera based imaging and another using X-ray film.

7.10 CCD camera

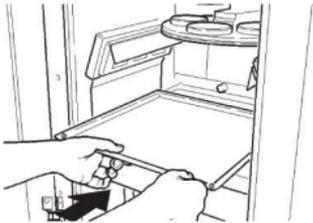Step	Action	Notes
1.	Place the blot, protein side up on a sample tray. 	The blot can be placed on a piece of plastic wrap, protein side up, to facilitate easy movement of the film on the sample tray.
2.	Place the sample tray in the CCD camera compartment and select suitable exposure time and/or function. 	Use the automatic exposure function or select exposure time manually. Recommended starting exposure time is 60 seconds. Increase or decrease exposure time depending on the obtained signal intensity.

7.11 X-ray film

Step	Action	Notes
1.	Place the blot with protein side down on to a fresh piece of plastic wrap, wrap the blots and gently smooth out any air bubbles.	
2.	Place the wrapped blot with protein side up in an X-ray film cassette.	Make sure there is no free detection reagent in the cassette; the film must not get wet.
3.	Place a sheet of X-ray film (Amersham Hyperfilm product range) on top of the membrane. Close the cassette and allow exposure. Suitable exposure start time is 1 minute.	This stage should be carried out in a dark room using red safe lights. Do not move the film while it is being exposed.
4.	Develop the film immediately and, on the basis of the signal intensity obtained, estimate exposure time for a second sheet of film.	

8. Additional information

8.1 Stripping and reprobing membranes

The complete removal of primary and secondary antibodies from the membrane is possible following the protocol outlined below. The membranes may be stripped and reprobed several times.

Step	Action	Notes
1.	Place the membrane in stripping buffer (100 mM 2-mercaptoethanol, 2% SDS, 62.5 mM Tris-HCl pH 6.7) and incubate at 50°C for 30 minutes with occasional agitation.	If more stringent conditions are required, the incubation can be performed at 70°C or for a longer time.
2.	Wash the membrane for 3 × 10 minutes in PBS-T or TBS-T at room temperature using large volumes of wash buffer. The membrane may be used immediately or stored in PBS-T or TBS-T at 2 to 8°C.	Membranes may be incubated with Amersham ECL Select detection reagent and exposed to film to ensure removal of antibodies.
3.	Block the membrane in a suitable blocking solution for 1 hour at room temperature.	
4.	Repeat the immunodetection protocol in Chapter 7, Protocol from Antibody probing to Image analysis.	

8.2 Determination of optimum antibody concentration

Due to the high signal intensity of the Amersham ECL Select detection reagent, optimization of antibody concentrations is recommended to ensure the best results. In general, very highly diluted primary and secondary antibodies are required with Amersham ECL Select detection reagent compared to standard chemiluminescent substrates. Outlined below are protocols for determining optimal antibody concentrations.

8.3 Dilution ranges

The following dilution ranges are recommended:

Antibody	Dilution range from 1 mg/ml stock solution
Primary	1:5000 - 1:30000
Secondary	1:100000 - 1:300000

8.4 Primary antibody optimization

Dot blotting is a quick and effective method of determining the optimum dilution of a primary antibody of unknown concentration. Alternatively, a Western blot can be prepared and then cut into several strips. It should be noted that some antibodies may require alternative blocking and washing steps to the ones suggested below.

Step	Action
------	--------

1. Spot different amounts of protein sample, preferably a dilution series, on to a PVDF or nitrocellulose membrane and allow to air dry. Alternatively, use a dot blot or slot blot manifold. Make one sample series for each dilution to be tested. **Note:** *PVDF membranes must be pre-wetted in methanol.*

Step	Action
2.	Incubate in blocking solution for 1 hour at room temperature with agitation.
3.	Rinse the membranes briefly with two changes of wash buffer.
4.	Cut the membrane to get each sample series on a separate membrane strip.
5.	Prepare different primary antibody solutions within the recommended antibody range. Incubate each membrane strip in antibody solution for 1 hour at room temperature with agitation.
6.	Briefly rinse the membrane with two changes of wash buffer. Wash the membrane by suspending it in wash buffer and agitate for 5 minutes in room temperature. Replace wash buffer at least 4 to 6 times.
7.	Dilute the secondary antibody (using only one concentration) and incubate the membranes for 1 hour at room temperature with agitation.
8.	Rinse blots in two changes of wash buffer, then wash 4 to 6 times in fresh changes of wash buffer.
9.	Detect using Amersham ECL Select detection reagent detailed in <i>Detection, on page 18</i> of the protocol. The antibody dilution which gives the best signal with the minimum background should be selected.

8.5 Secondary antibody optimization

Step	Action
1.	Spot different amounts of protein sample, preferably a dilution series, on to a PVDF or nitrocellulose membrane and allow to air dry. Alternatively, use a dot blot or slot blot manifold. Make one sample series for each dilution to be tested. Note: <i>PVDF membranes must be pre-wetted in methanol.</i>
2.	Incubate in blocking solution for 1 hour at room temperature with agitation.
3.	Incubate in diluted primary antibody (optimized concentration) for 1 hour at room temperature with agitation.
4.	Briefly rinse the membrane with two changes of wash buffer. Wash the membrane by suspending it in wash buffer and agitate for 5 minutes in room temperature. Replace wash buffer at least 4 to 6 times.
5.	Cut the membrane to get each sample series on a separate membrane strip.
6.	Prepare different secondary antibody solutions within the recommended antibody range. Incubate each membrane strip in antibody solution for 1 hour at room temperature with agitation.
7.	Briefly rinse the membrane with two changes of wash buffer. Wash the membrane by suspending it in wash buffer and agitate for 5 minutes in room temperature. Replace wash buffer at least 4 to 6 times.
8.	Detect using Amersham ECL Select detection reagent detailed in <i>Detection, on page 18</i> of the protocol. The antibody dilution which gives the best signal with minimum background should be selected.

9. Troubleshooting guide

Problems	Possible causes / remedies
No signal	<ul style="list-style-type: none">• Non-detectable amounts of target protein.• Primary antibody is not binding to target protein, which may be due to bad quality and/or unspecific primary antibody.• Incorrect species of secondary antibody has been used.• PVDF membrane not pre-wetted in methanol.• Check that transfer equipment is working properly and that the correct procedure has been followed.• Check protein transfer by staining the membrane and/or gel.• Confirm transfer efficiency by using pre-stained Rainbow marker.• Some proteins may be affected by the treatments required for electrophoresis.• Detection reagents do not function properly.<ul style="list-style-type: none">- To test the detection reagent activity, in a darkroom prepare 1 to 2 ml of detection reagent working solution in a clear test tube. Add 1 μl of undiluted HRP-conjugated antibody solution. The solution should immediately emit a visible blue light that fades during the next several minutes.• Incorrect storage of Amersham ECL Select detection reagent may cause a loss of signal. Bacterial growth inhibit the reagent.

Problems	Possible causes / remedies
Weak signal	<ul style="list-style-type: none"> • Transfer efficiency may have been poor. • Insufficient protein was loaded on to the gel. • The concentration of primary and secondary antibodies could be too low; optimization is required. • Bad quality and/or unspecific primary antibody. • Exposure time may have been too short.
Excessive, diffuse signal	<ul style="list-style-type: none"> • Too much protein was loaded on to the gel. • The concentrations of primary and secondary antibodies could be too high; optimization is required.
White (negative) bands on the film	<ul style="list-style-type: none"> • Negative bands generally occur when protein target is in excess and antibody concentrations are too high. The effect is caused by substrate depletion. <ul style="list-style-type: none"> - Load less amount of protein. - Dilute both primary and secondary antibody further.
Uneven, spotted background	<ul style="list-style-type: none"> • Areas of the blot may have dried during some of the incubations. • Incorrect handling can lead to contamination on the blots and/or membrane damage which may cause non-specific signal. • The blocking agent is not completely dissolved in the buffer. • Insufficient washing. <ul style="list-style-type: none"> - Add additional washing steps.

Problems	Possible causes / remedies
High backgrounds	<ul style="list-style-type: none"> • Too high concentrations of primary and secondary antibodies; optimization is required. • Insufficient washing. <ul style="list-style-type: none"> - Use sufficient amount of wash buffer and add additional washing steps. • Transfer and incubation buffers may have become contaminated and require replacing. <ul style="list-style-type: none"> - Always use fresh solutions • Insufficient blocking. • The blocking agent used was not freshly prepared or was too dilute or was incompatible with the application. • The level of Tween used in the blocking agent was not sufficient for the application performed. • The membrane was allowed to dry during some of the incubations. • Poor gel quality. • Unspecific and bad quality of antibodies. • The film detection of the signal was allowed to over expose. • The level of signal is so high that the film has become completely overloaded. • Non compatible products.

10. Related products

This chapter presents a subset of related products. For more information, refer to www.gelifesciences.com/ecl.

10.1 Sample preparation

Product	Quantity	Code no.
SDS-PAGE Clean-up kit	50 samples	80-6484-70
Mammalian Protein Extraction Buffer	1 × 500 ml	28-9412-79
2-D Quant Kit	500 assays	80-6483-56

10.2 Molecular weight markers

Product	Quantity	Code no.
Amersham Low-Range Rainbow Molecular Weight Markers	250 µl	RPN755E
Amersham High-Range Rainbow Molecular Weight Markers	250 µl	RPN756E
Amersham Full-Range Rainbow Molecular Weight Markers	250 µl	RPN800E
Amersham ECL DualVue Western Blotting Markers	1 pack (25 loadings)	RPN810
Amersham ECL Plex™ Fluorescent Rainbow Markers	120 µl	RPN850E
Amersham ECL Plex Fluorescent Rainbow Markers	500 µl	RPN851E

10.3 Gel electrophoresis equipment

Product	Quantity	Code no.
Gel electrophoresis		
Amersham ECL Gel Box	1	28-9906-08
Amersham ECL Gel 10%, 10 wells	10	28-9898-04
Amersham ECL Gel 12%, 10 wells	10	28-9898-05
Amersham ECL Gel 4-12%, 10 wells	10	28-9898-06
Amersham ECL Gel 8-16%, 10 wells	10	28-9898-07
Amersham ECL Gel 4-20%, 10 wells	10	28-9901-54
Amersham ECL Gel 10%, 15 wells	10	28-9901-55
Amersham ECL Gel 12%, 15 wells	10	28-9901-56
Amersham ECL Gel 4-12%, 15 wells	10	28-9901-57
Amersham ECL Gel 8-16%, 15 wells	10	28-9901-58
Amersham ECL Gel 4-20%, 15 wells	10	28-9901-59
Amersham ECL Gel 10%, 2 wells	10	28-9901-60
Amersham ECL Gel 12%, 2 wells	10	28-9901-61

Product	Quantity	Code no.
Gel electrophoresis		
Amersham ECL Gel 4-12%, 2 wells	10	28-9901-62
Amersham ECL Gel 8-16%, 2 wells	10	28-9901-63
Amersham ECL Gel 4-20%, 2 wells	10	28-9901-64
Amersham ECL Gel 10%, 10 wells	2	28-9898-08
Amersham ECL Gel 12%, 10 wells	2	28-9898-09
Amersham ECL Gel 4-12%, 10 wells	2	28-9901-51
Amersham ECL Gel 8-16%, 10 wells	2	28-9901-52
Amersham ECL Gel 4-20%, 10 wells	2	28-9901-53
Power Supplies		
EPS 301 Power Supply	1	18-1130-01
EPS 2A201 Power Supply	1	28-9202-14

10.4 Transfer equipment

Product	Quantity	Code no.
Tank transfer units		
TE 22 Mini Tank Transfer Unit	1	80-6204-26
ECL Semidry Blotters		
TE 70 Semi-Dry Transfer Unit, 14 × 16 cm	1	80-6210-34
TE 70 PWR Semi-Dry Transfer Unit, 14 × 16 cm ¹	1	11-0013-41
TE 77 Semi-Dry Transfer Unit, 21 × 26 cm	1	80-6211-86
TE 77 PWR Semi-Dry Transfer Unit, 21 × 26 cm	1	11-0013-42

10.5 Blotting equipment

Product	Quantity	Code no.
Blotting paper		
Hybond blotting paper (20 × 20 cm)	100 sheets	RPN6101M
3MM Chr 20 × 20 cm	100 sheets	3030-861

Product	Quantity	Code no.
Membranes		
Amersham Protran Supported 0.2 NC (20 × 20 cm)	25 sheets	10600053
Amersham Protran Supported 0.2 NC (8 × 9 cm)	25 sheets	10600099
Amersham Hybond LFP 0.2 PVDF (20 × 20 cm)	10 sheets	10600060
Amersham Hybond LFP 0.2 PVDF (8 × 9 cm)	25 sheets	10600102
Amersham Hybond 0.2 PVDF (20 × 20 cm)	25 sheets	10600057
Amersham Hybond 0.2 PVDF (8 × 9 cm)	25 sheets	10600101

10.6 Blocking agents

Product	Quantity	Code no.
Amersham ECL Blocking Agent	40 g	RPN2125
Amersham ECL Prime Blocking Agent	40 g	RPN418

10.7 Amersham ECL HRP-linked secondary antibodies

Product	Quantity	Code no.
Amersham ECL Mouse IgG,HRP-Linked Whole Ab (from sheep)	1 ml	NA931-1ML
Amersham ECL Human IgG, HRP-Linked Whole Ab (from sheep)	1 ml	NA933-1ML
Amersham ECL Rabbit IgG, HRP-Linked Whole Ab (from donkey)	1 ml	NA934-1ML
Amersham ECL Mouse IgG,HRP-Linked F(ab)2 fragment (from sheep)	1 ml	NA9310-1ML
Amersham ECL Rabbit IgG, HRP-Linked F(ab)2 fragment (from donkey)	1 ml	NA9340-1ML
Amersham ECL Plex™ goat- α -mouse IgG-Cy2	150 μ g	28-9011-08
Amersham ECL Plex goat- α -rabbit IgG-Cy2	150 μ g	28-9011-10
Amersham ECL Plex goat- α -rabbit IgG-Cy3	150 μ g	28-9011-06
Amersham ECL Plex goat- α -mouse IgG-Cy3	150 μ g	PA43009
Amersham ECL Plex goat- α -rabbit IgG-Cy5	150 μ g	PA45011
Amersham ECL Plex goat- α -mouse IgG-Cy5	150 μ g	PA45010

10.8 Detection reagents

Product	Quantity	Code no.
Amersham ECL Select Western Blotting Detection Reagent	for 1000 cm ²	RPN2235
Amersham ECL Prime Western Blotting Detection Reagent	for 1000 cm ²	RPN2232
Amersham ECL Western Blotting Detection Reagents	for 1000 cm ²	RPN2109
Amersham ECL Western Blotting Detection Reagents	for 4000 cm ²	RPN2106
Amersham ECL Western Blotting Detection Reagents	for 6000 cm ²	RPN2134

10.9 ECL Plex CyDye conjugated antibodies

Product	Quantity	Code no.
Amersham ECL Plex Western Blotting Combination Pack (Cy3, Cy5, Hybond ECL)	1	RPN998
Amersham ECL Plex Western Blotting Combination Pack (Cy3, Cy5, Hybond LFP) for two slab gels	1	RPN999

10.10 X-ray films

Product	Quantity	Code no.
Amersham Hyperfilm ECL (5 × 7 inches)	50 sheets	28-9068-35
Amersham Hyperfilm ECL (18 × 24 cm)	50 sheets	28-9068-36
Amersham Hyperfilm ECL (8 × 10 inches)	50 sheets	28-9068-38

10.11 Imaging systems

Product	Quantity	Code no.
ImageQuant LAS 500	1	29-0050-63

10.12 Software and accessories

Product	Quantity	Code no.
CD and getting started:		
ImageQuant TL and IQTL SecurTy Software package (with Getting Started Guide)		28-9380-94
Licenses for ImageQuant TL only:		
ImageQuant TL, single user license		28-9236-62
Licenses for ImageQuant TL and IQTL SecurTy:		
ImageQuant TL and ImageQuant TL SecurTy	1-user	28-9332-73

GE Healthcare offices:

GE Healthcare UK Limited
Amersham Place
Little Chalfont, Buckinghamshire,
HP7 9NA, UK

GE Healthcare Bio-Sciences AB
Björkgatan 30, 751 84 Uppsala,
Sweden

GE Healthcare Europe GmbH
Munzinger Strasse 5, D-79111 Freiburg,
Germany

GE Healthcare Bio-Sciences Corp.
100 Results Way, Marlborough,
MA 01752
USA

GE Healthcare Dharmacon.
2650 Crescent Drive, Lafayette,
CO 80026
USA

Hyclone Laboratories, Inc.
925 W 1800 S, Logan
UT 84321
USA

GE Healthcare Japan Corporation
Sanken Bldg. 3-25-1, Hyakunincho,
Shinjuku-ku, Tokyo 169-0073,
Japan

For your local office contact information, visit
www.gelifesciences.com/contact

GE Healthcare UK Limited
Amersham Place
Little Chalfont, Buckinghamshire,
HP7 9NA, UK

<http://www.gelifesciences.com>



imagination at work